

Forschungsinstitut für Resonanzphänomene

Olaf Baumunk -- Bioplasmatist

Schwand 9 --- D 79837 Häusern

Tel: 0176 - 42640640 -- E-Mail: baumunk52@aol.de

Aschoff-Test: BioRing by SWISS HARMONY

April, 16th 2016



The Aschoff-Test is an approved test method protected by patent in the Federal Patent Department of Germany. In the Aschoff-Test the skin resistance of the ten ting points of the proband`s left hand are metered with a device called the BIO OHM TESTER.

The higher the skin resistance data is, the worse is the bio-energetical condition of the proband.


The standard value of a healthy person runs at about 40 kilo ohm. But this value is generally not achieved. Usually the value is up to 60 - 70 kilo ohm.

MP 1 - 10 are the 10 metering points on the fingers.

The first measurement is taken **without putting any strain** on the proband.
(blue line in the graph)

The second measurement i staken **with added strain on the proband but without the BioRing.** (red line in the graph)

The third measurement is taken **with added strain on the proband but with the BioRing.** (grey line in the graph)

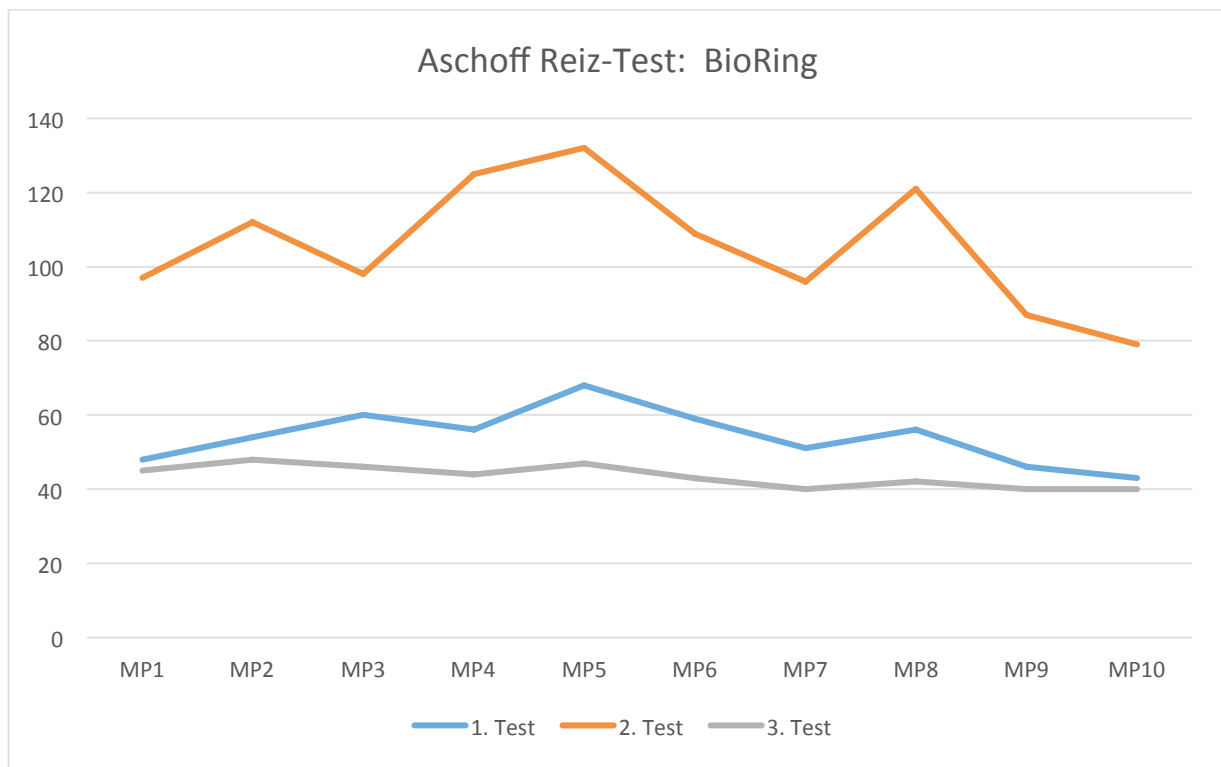

The outcome:

The first reading shows only a slight divergence of the general skin resistance value of 40 kilo ohm. This is probably based on the fact, that the proband has been continuously carrying the Body Card since the last test from the day before. This fact has very likely stabilized the bio-energetic field of the proband. 3 hours before this BioRing- test was done, the Body Card was removed from the proband but his energy-field somehow remained stable, which indicates a general stabilization of the proband's bio-energetic body field by continuous use of SWISS HARMONY devices.

At the second reading the proband is exposed to extensive electromagnetic contamination in form of the high frequency radiation from two mobile phones and the low frequency electromagnetic field of a current-carrying electrical wire. The red line in the graph shows a significant increase of the skin resistance,

which implies a strong health risk.

The measured data of the third reading is remarkable low even though the proband is still exposed to the same electromagnetic contamination as at the second reading -- but with the difference of carrying the BioRing on his finger. The measured data almost reach the normal value of 40 kilo ohm. This allows only one conclusion: The continuous application of SWISS HARMONY products leads to a general stabilization of the user's bio-energetic body field.

The BioRing made by SWISS HARMONY generates a healthful energy field, which completely neutralizes the bad effects from electromagnetic and other pathogenic energy fields. The BioRing by SWISS HARMONY is a very valuable bio-energetic device.